



A) UV

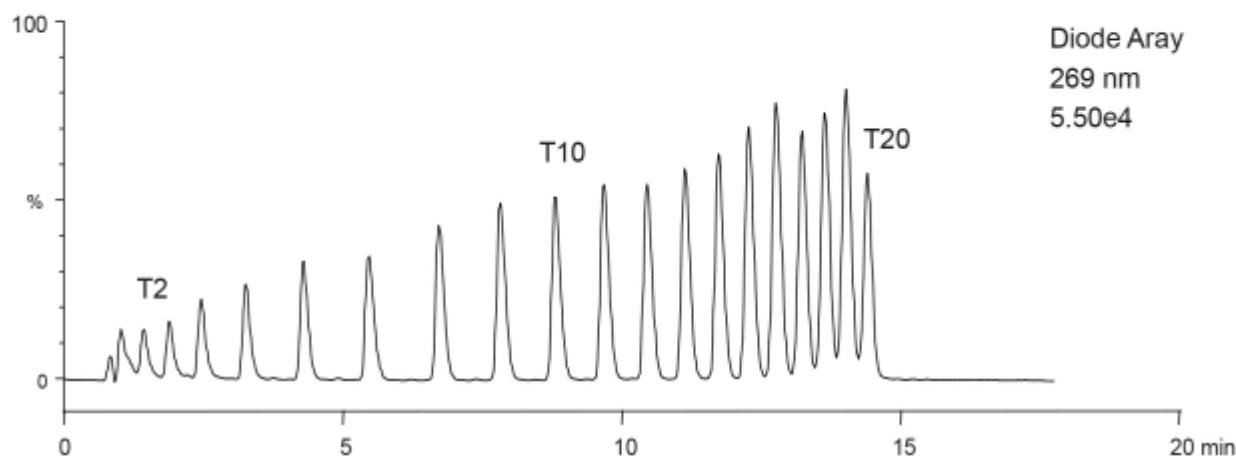

B) MS

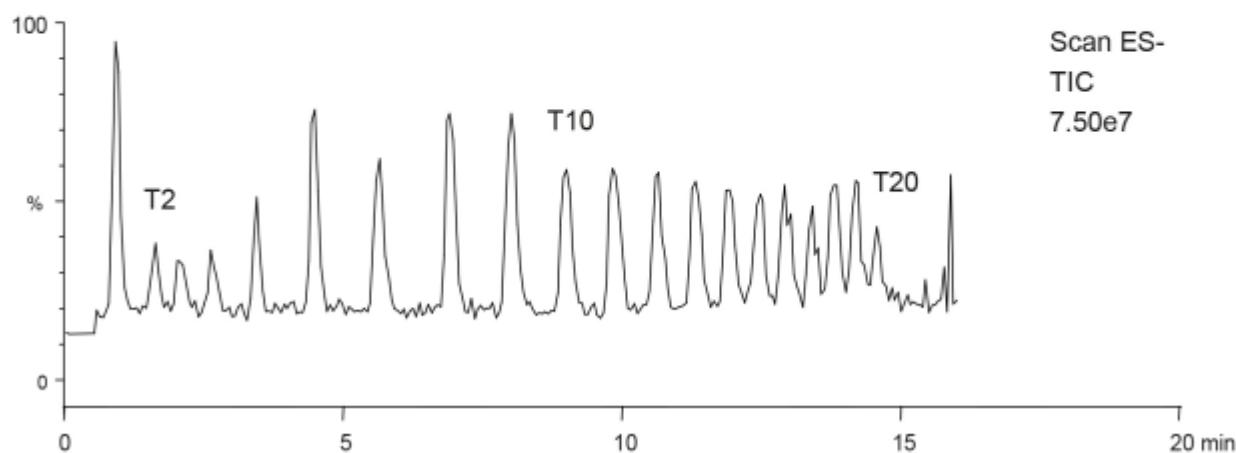

Column	: Hydrosphere C18 (3 µm, 12 nm) 50 X 2.0 mmI.D.
Eluent	: A) 5 mM di-n-butylamine - acetic acid (pH 6.0) B) 5 mM di-n-butylamine - acetic acid (pH 6.0) / methanol (20/80) 42-70% B (0-20 min)
Flow rate	: 0.2 mL/min
Temperature	: 35 °C
Detection	: A) UV at 269 nm B) ESI negative-mode
Injection	: 5 µL (5 nmol/mL)